Depletion of Phospholipid Matrix Interference when Dealing with Small Volume Plasma Samples

Craig Aurand, David Bell, and Hillel Brandes

Supelco, Div. of Sigma-Aldrich, Bellefonte, PA 16823 USA



sigma-aldrich.com

T410128

© 2010 Sigma-Aldrich Co. All rights reserved.

SIGMA-ALDRICH®

Introduction

- Sample preparation of small volume plasma samples can be restrictive due to the limited volume of available plasma.
- Mouse studies, plasma samples are limited to 30 µL or less.
- Traditional solid phase extraction techniques limited due to large hold up volumes.
- Often limited to liquid-liquid protein precipitation resulting in a high degree of matrix interference.
- Major concern in developing bioanalytical methods is addressing matrix effects.
- Co-extracted interferences directly affect the quantitation of analytes.
- Matrix build up that leads to irregularities in quantitation.
- Gradient elution often required for matrix elution…time consuming.


© 2010 Sigma-Aldrich Co. All rights reserved.

Experimental

- In this study, comparisons are made between standard protein precipitation methods along with sample preparation by HybridSPE®-PPT small volume technique for the recovery of methadone and metabolites from plasma samples along with effective matrix removal.
- Spiked rat plasma samples with methadone and metabolites EDDP and EMDP processed by standard protein precipitation compared against HybridSPE-Small Volume 96-well plate.
- The analysis was conducted on an Agilent 1200SL Rapid Resolution system coupled to an Agilent 6210 TOF LC/MS. Chromatographic separation was performed on the Ascentis® Express RP-Amide.
- The high sensitivity of methadone and metabolites enable for direct small volume injection of the processed sample without the need for evaporation or reconstitution.
- EDDP, Cerilliant E-012, E-022 (as pyrolinium); Methadone, Cerilliant M-007, M-019; EMDP, Cerilliant E-057 (as free base).

© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 1. Chromatographic Conditions

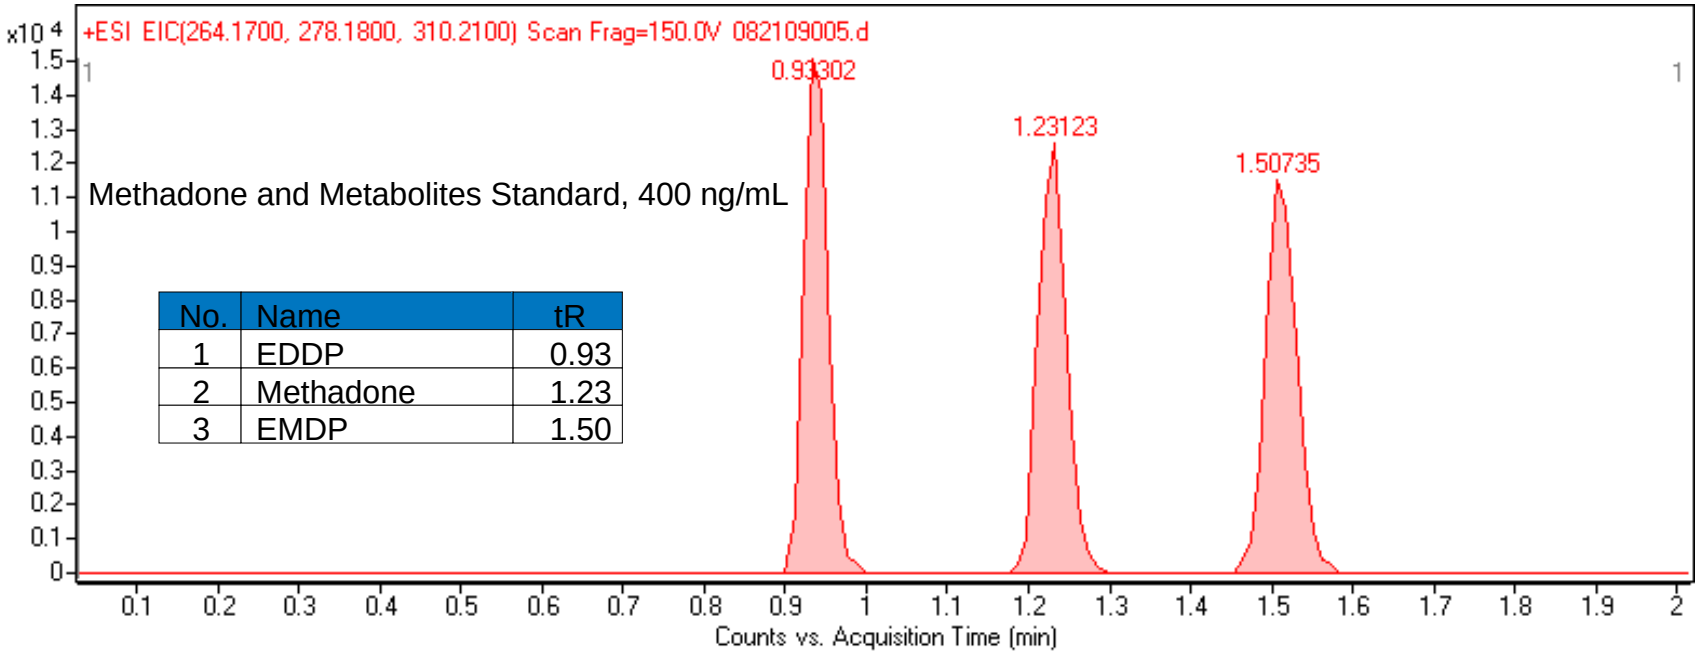

No.	Name	tR
1	EDDP	0.93
2	Methadone	1.23
3	EMDP	1.50

column: Ascentis® Express RP Amide, 10 cm x 2.1 mm I.D., 2.7 µm particles, (53913-U)
mobile phase: 10 mM ammonium formate (65:35 water:acetonitrile) pH 3.6
flow rate: 0.4 mL/min.
system pressure: 275 bar
temp.: 35 °C
det.: ESI+, 1.5 spectra/sec, 6309 transients/spectra
inj.: 0.5 µL
instrument: Agilent 1200SL Rapid Resolution, Agilent 6210 TOF LC/MS

© 2010 Sigma-Aldrich Co. All rights reserved.

Phospholipid Monitoring

Lysophosphatidylcholines:	m/z
1-palmitoyl-2-hydroxy-sn-glycero-3-phosphocholine	496.3
1-stearoyl-2-hydroxy-sn-glycero-3-phosphocholine	524.3

Glycerophosphocholines:	m/z
1-hexadecanoyl-2-(9Z,12Z-octadecadienoyl)-sn-glycero-3-phosphocholine	758.5
glycerophosphocholine 36:2	786.5
1-(9Z,12Z-octadecadienoyl)-2-(5Z,8Z,11Z,14Z-eicosatetraenoyl)-sn-glycero-3-phosphocholine	806.5
1-stearoyl-2-arachidonoyl-*sn*-glycero-3-phosphocholine	810.5

© 2010 Sigma-Aldrich Co. All rights reserved.

Sample Preparation

Standard Solutions: Standard solutions were prepared from a stock standard in (3:1) 1% formic acid acetonitrile:water at a level of 1, 10, 20, 50, 100, 200, 500 ng/mL.

Plasma: Rat plasma stabilized with K_2EDTA was acquired from Lampire Biological Laboratories, (Pipersville PA). Plasma was spiked directly from stock standard to a level of 20, 50, 100, 400, 300 ng/mL.

Standard Protein Precipitation: apply 20 µL of plasma to centrifuge vial, followed by 60 µL of 1% formic acid acetonitrile. Agitate via vortex for 1 minute, place into centrifuge for 2 minutes at 15000 rpm. Collect supernatant and analyze directly.


HybridSPE-small volume Plasma Samples: apply 20 µL of plasma to plate, followed by 60 µL of 1% formic acid acetonitrile. Agitate via vortex for 1 minute, place on vacuum manifold and apply 10”Hg vacuum for 2 minutes. Collect filtrate and analyze directly.

Collection Plate: Eppendorf 150 µL conical with mylar cover.

© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 2. Lewis Acid Base Strength Scale

Lewis Base	rel. Strength on Zirconia
Hydroxide	Strongest
Phosphate	
Fluoride	
Citrate	
Sulfate	
Acetate	
Formate	
Chloride	Weakest

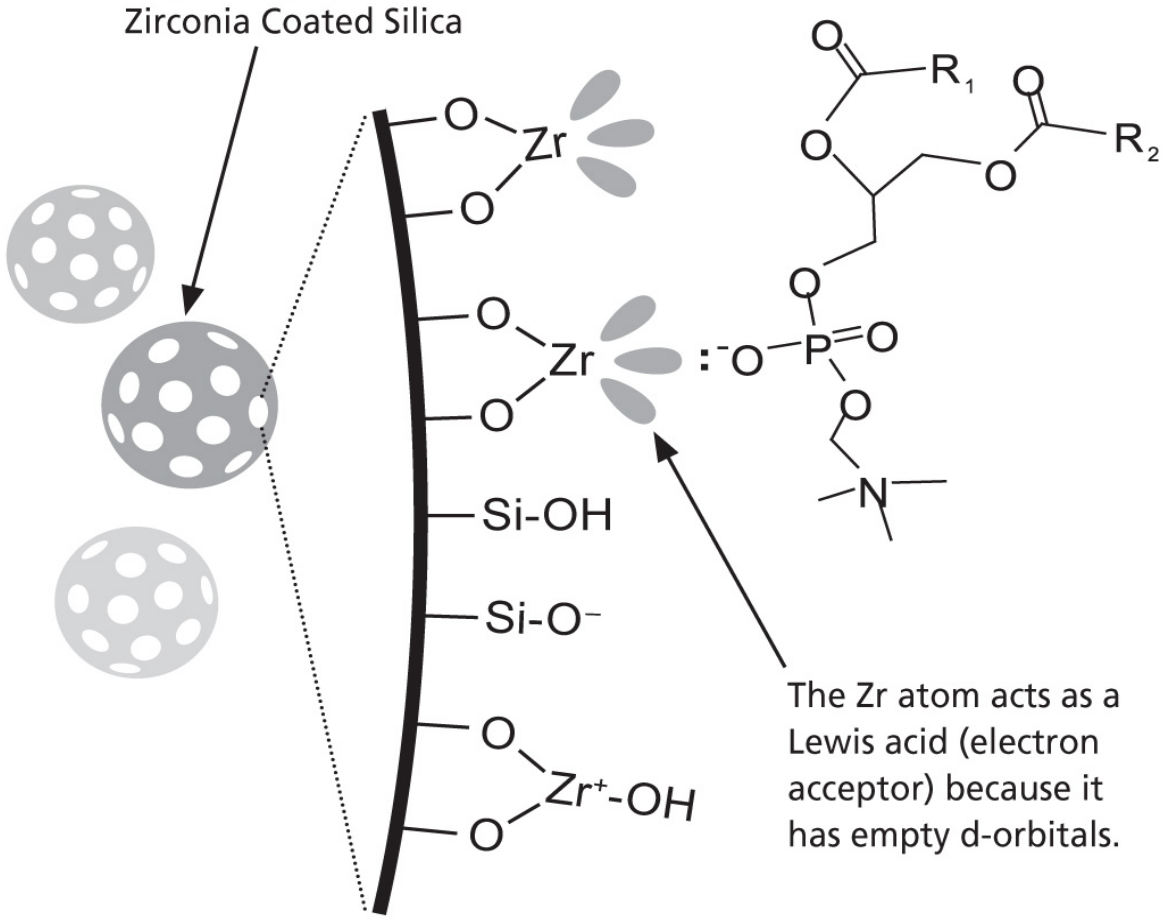


Interaction between a representative phospholipid and the zirconium surface of the HybridSPE-PPT particle via Lewis acid-base interaction.

© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 3. Crash Solvents and Additives

Precipitated Plasma Sample Composition


- Modifier (1% formic acid) mitigate lewis acid base interaction between chelation/ acidic compounds.
- Modifier (formic acid, ammonium formate) acts to disrupt ion-exchange with surface silanols.
- High organic content (75%+) acts as strong solvent when related to hydrophobic retention (acetonitrile, methanol).
- Aqueous content (25%) is strong solvent when related to HILIC retention.

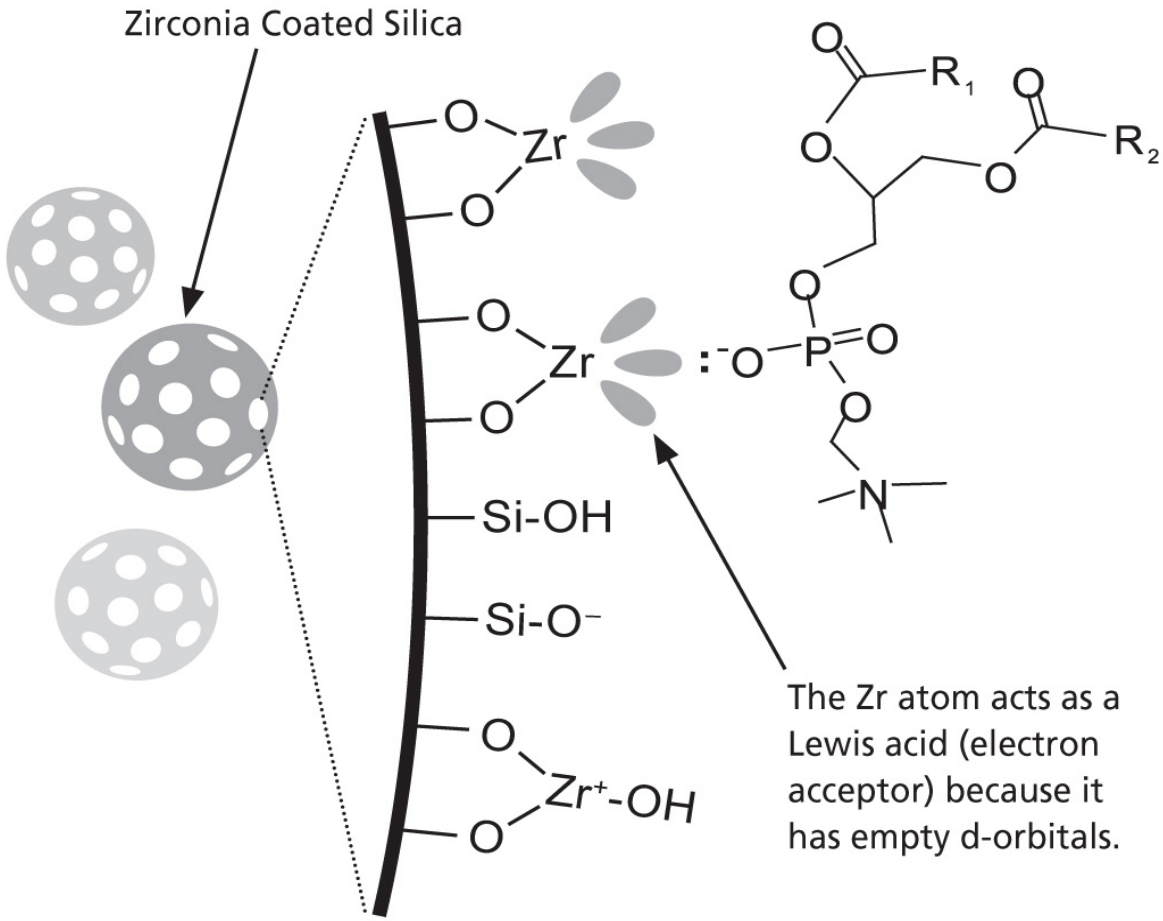


© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 4. *In-Well* Protein Precipitation Schematic

15 mg Zirconia-Coated Silica Bed

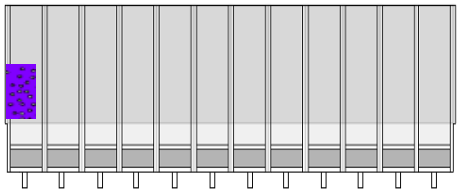




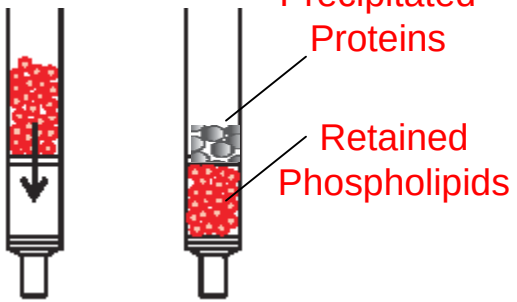

1) Precipitate Proteins: Add 20 µL plasma/serum followed by 60 µL 1% formic acid in acetonitrile. Add I.S. as necessary. Note: the upper PTFE frit keeps plasma from dripping through packed-bed prematurely.

2) Mix by vortexing HybridSPE plate or by aspirating/dispensing pipette tip.

3) Apply vacuum. Packed-bed filter/frit assembly acts as a depth filter for the concurrent physical removal of precipitated proteins and chemical removal phospholipids.



Recovery volume 40-50 µL

4) Resulting filtrate/eluate is depleted of proteins and phospholipids and ready for immediate LC-MS-MS analysis.

© 2010 Sigma-Aldrich Co. All rights reserved.

Experimental (contd.)

- Each spiked level sample was prepared n=8 for both sample prep techniques.
- Samples processed using the HybridSPE-Small Volume technique were collected directly into an Agilent low volume 96-well collection plate, average sample volume recovery from the plate was 40 µL.
- To ensure sufficient sample was drawn up by the injector, the auto sampler was set for bottom well sensing.
- Samples were assayed for content of methadone and metabolites along with matrix monitoring for phospholipids.
- Lyso and glycerophospholipids were monitored as a representative phospholipids matrix ions.

© 2010 Sigma-Aldrich Co. All rights reserved.

Injection Series

First Series: Calibration Standards

Level 1, 10, 20, 50, 100, 200, 500 ng/mL, n=8 for each level

Second Series: Spiked Plasma Samples HybridSPE

Level of 20, 50, 100, 200, 300 ng/mL, n=8 for each level


Third Series: Spiked Plasma Samples Protein Precipitation

Level of 20, 50, 100, 200, 300 ng/mL, n=8 for each level

Injections made in order of increasing concentration, blank injection performed between sample prep techniques. Sever signal suppression was observed for protein precipitation technique. Conversely, signal response very consistent for samples prepared using HybridSPE technique.

© 2010 Sigma-Aldrich Co. All rights reserved.


Figure 5. Calibration Table

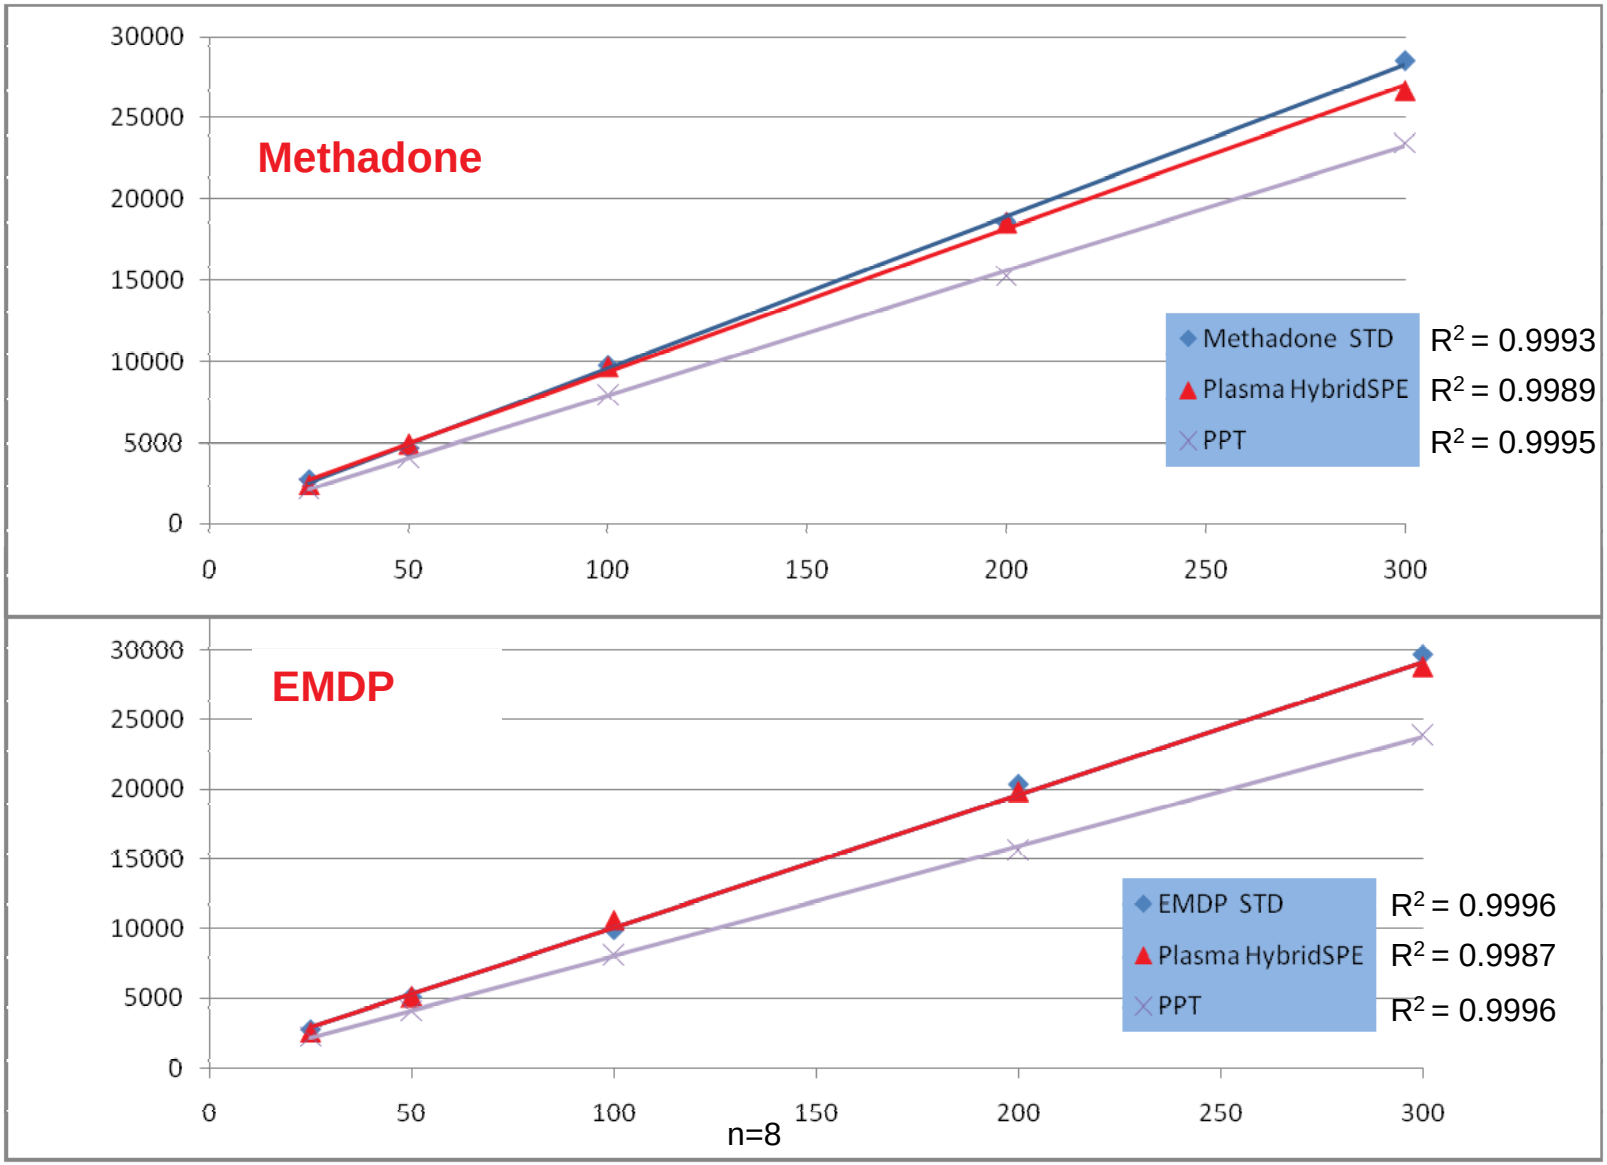

© 2010 Sigma-Aldrich Co. All rights reserved.


SIGMA-ALDRICH®

Figure 5. Calibration Table (contd.)

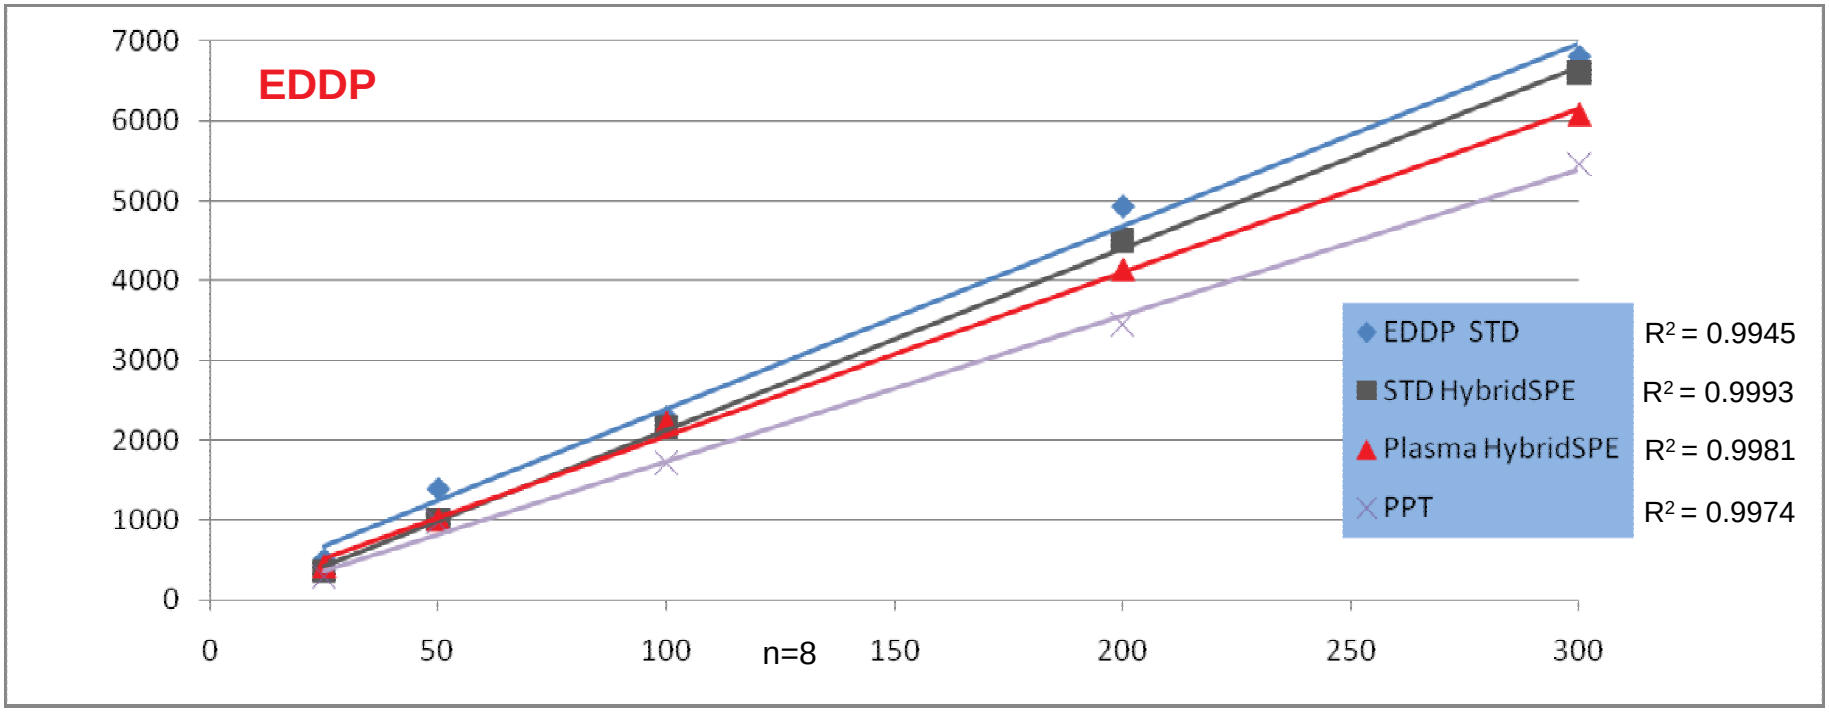

© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 6. Phospholipid Buildup on Column from Protein Precipitation Method

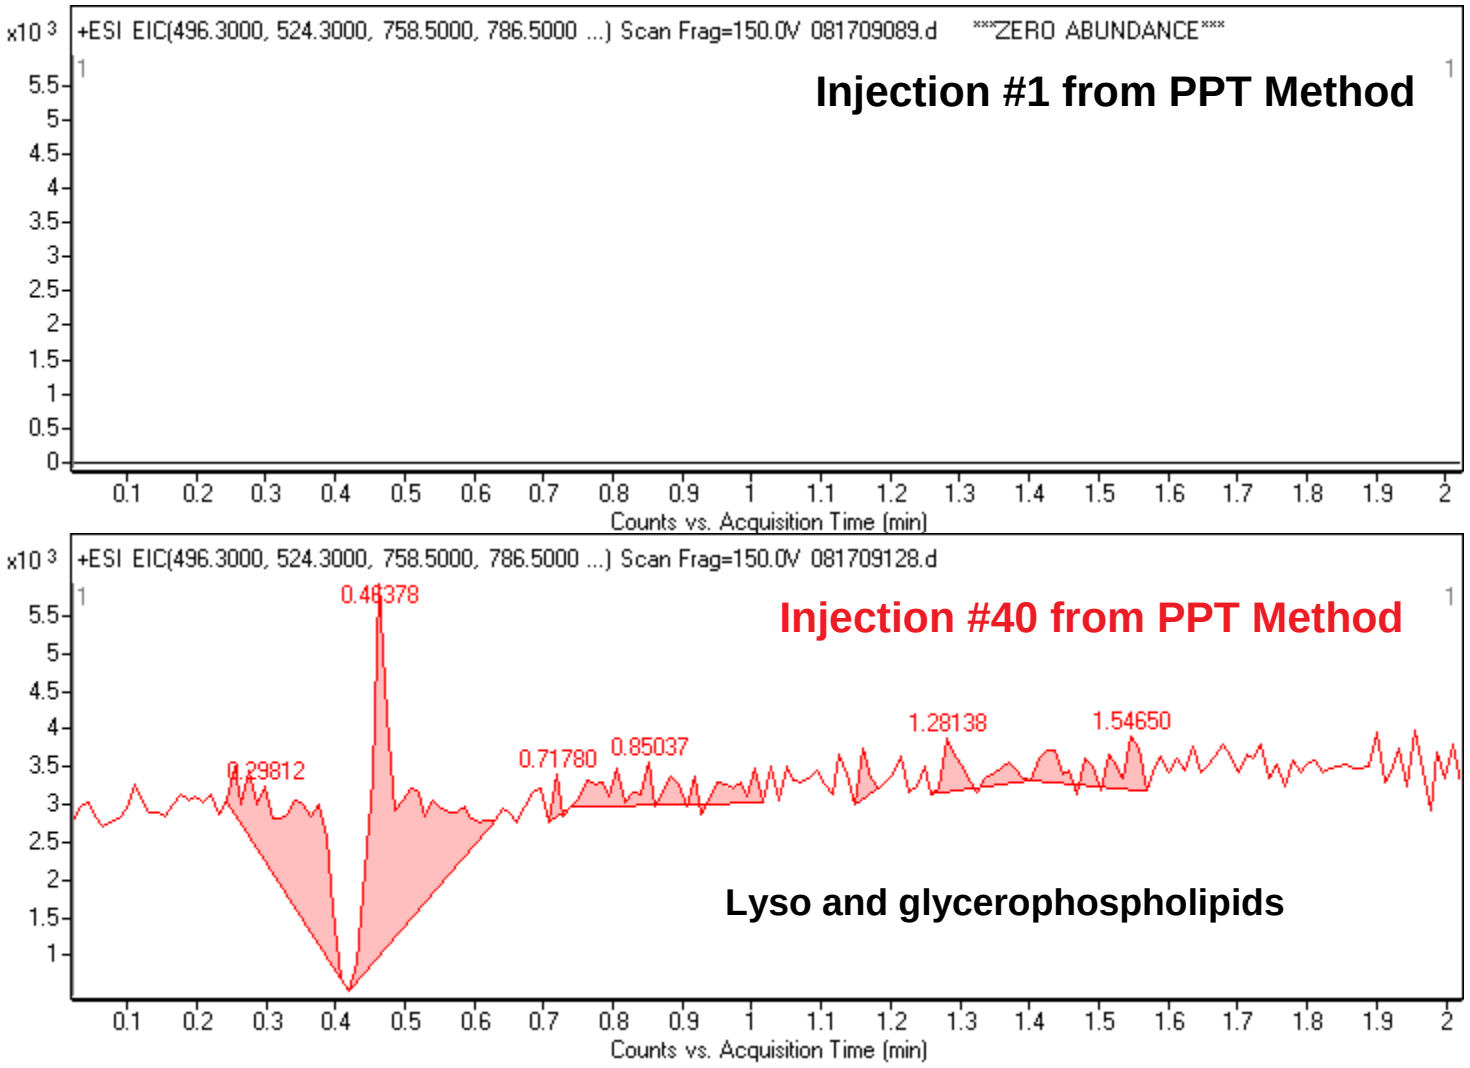


© 2010 Sigma-Aldrich Co. All rights reserved.

SIGMA-ALDRICH®

Figure 7. Overlay of HybridSPE-Small Volume and Protein Precipitation Samples

No.	Name	tR
1	EDDP	0.93
2	Methadone	1.23
3	EMDP	1.50

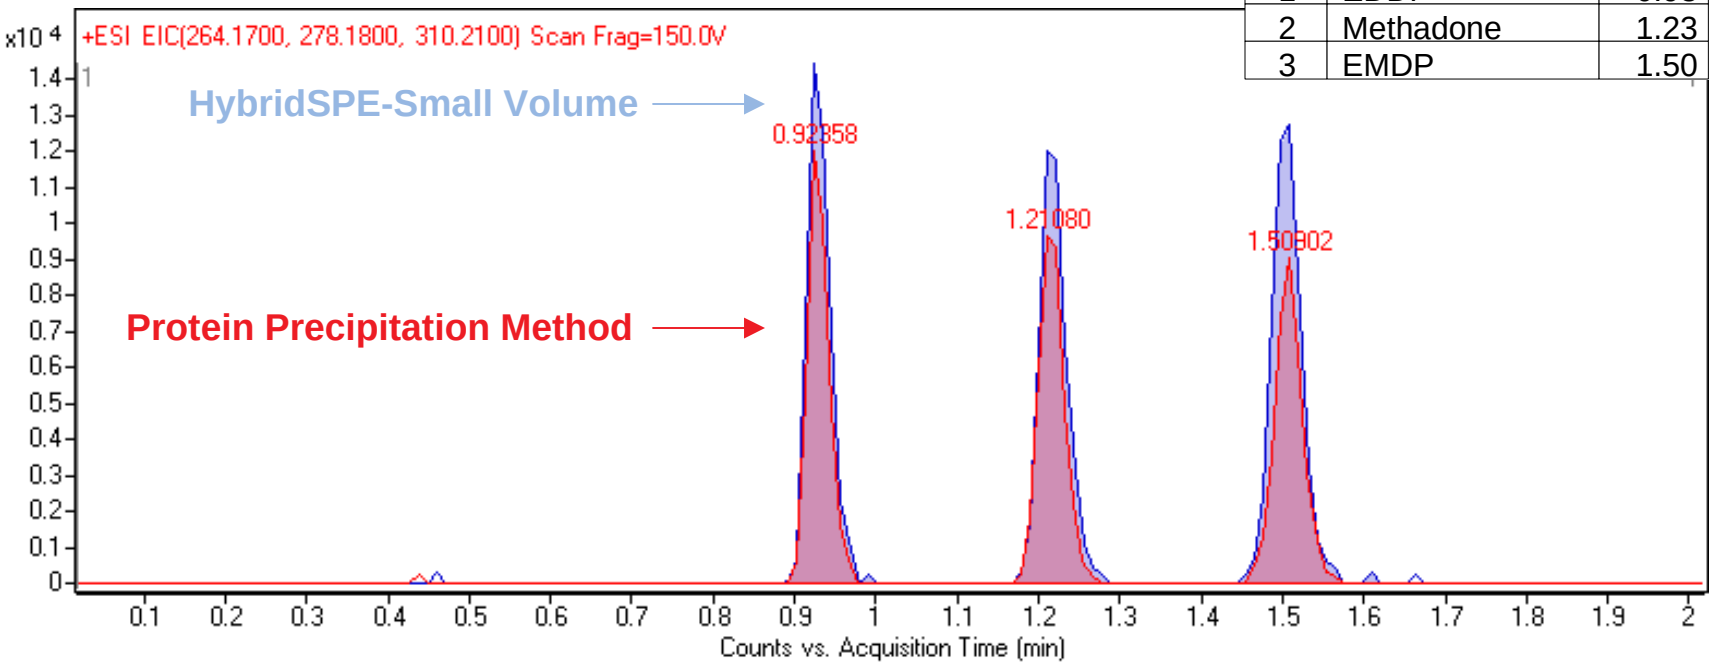

- Signal suppression observed even at highest spike level.
- Dramatic signal reduction over short number of samples for protein precipitation technique. Phospholipid buildup causing signal suppression of analytes from protein precipitation technique.

© 2010 Sigma-Aldrich Co. All rights reserved.


Long Term Injection Series

Continuation of study, this time set up as long term bioanalytical assay.

- Set up as standard bioanalytical method
- Spiked control samples run every 40 sample injection
- Control spiked at 100 ng/mL level
- Experiment conducted over a 250 injection series
- Control response was plotted
- Comparison between sample prep techniques


© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 8. Phospholipid Buildup on Column from Protein Precipitation Method

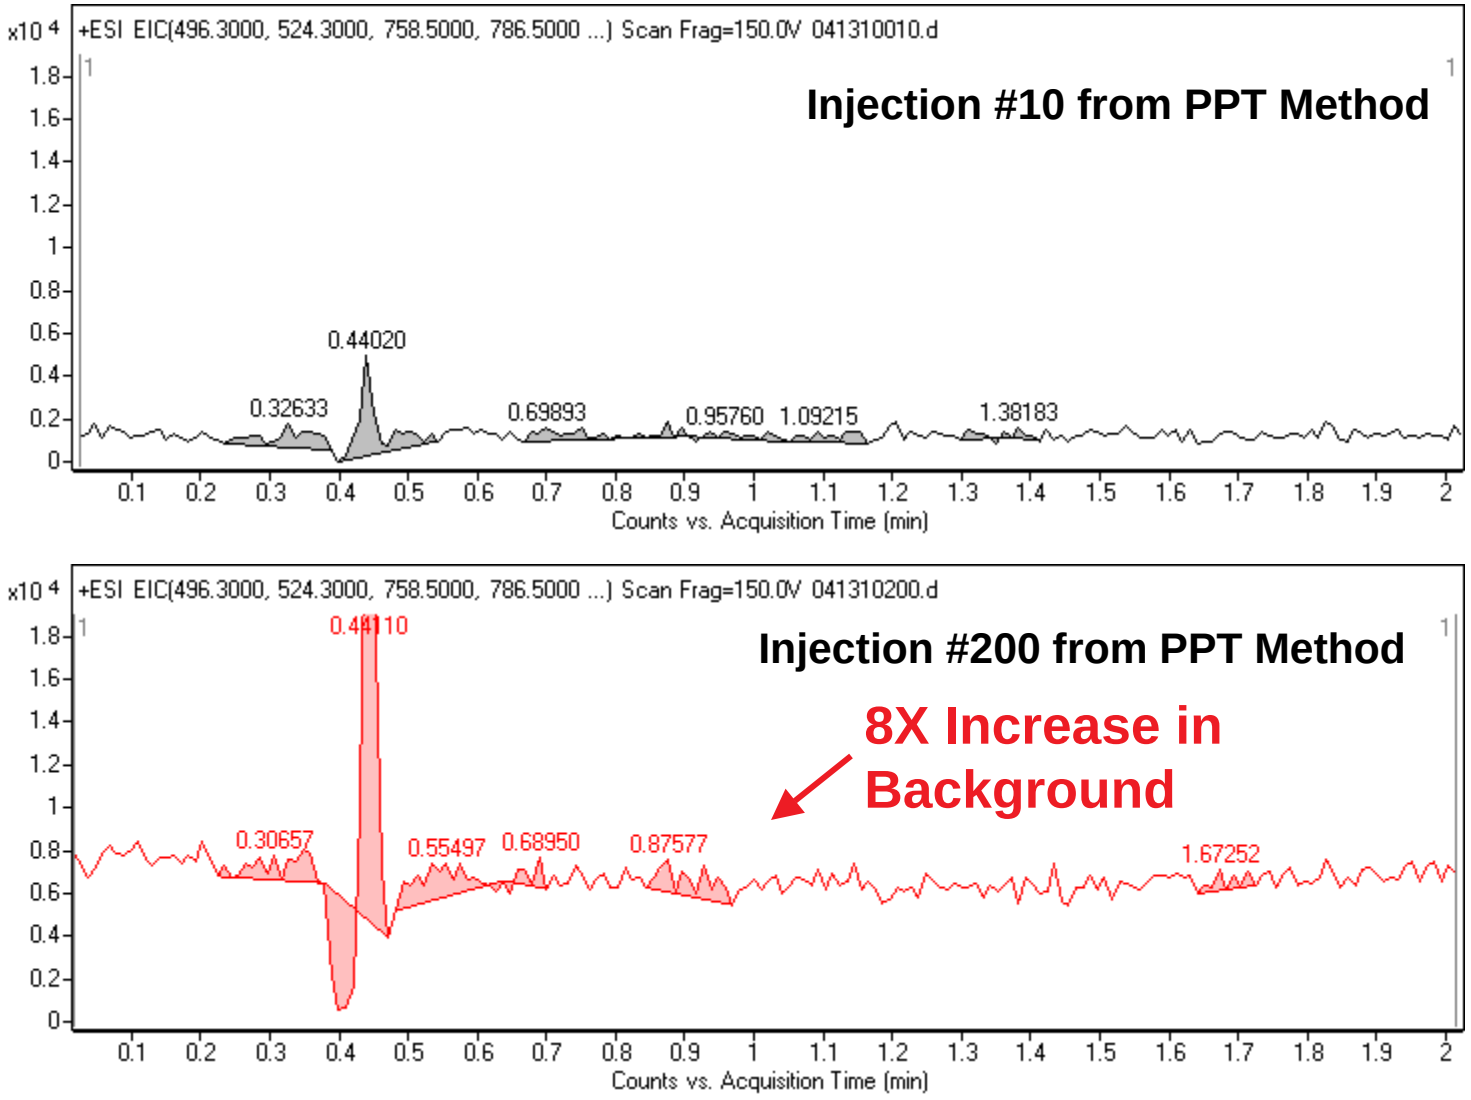


© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 9. Phospholipid Buildup from HybridSPE

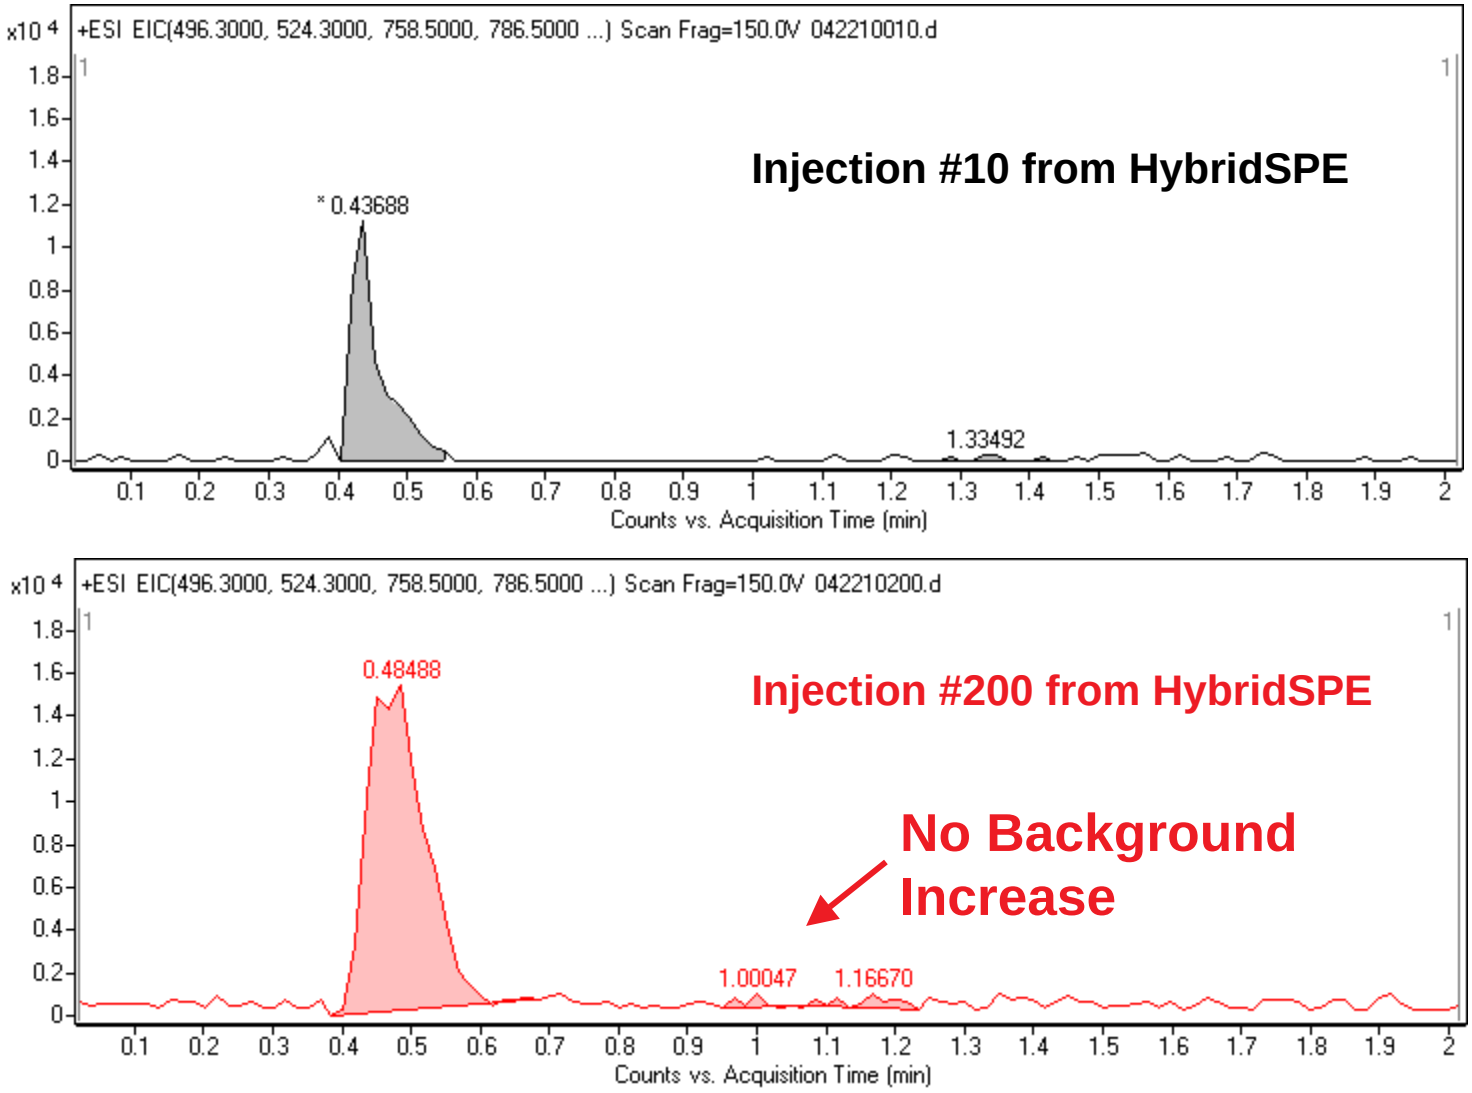

© 2010 Sigma-Aldrich Co. All rights reserved.

Figure 10. Ionization Effect of Phospholipid Buildup

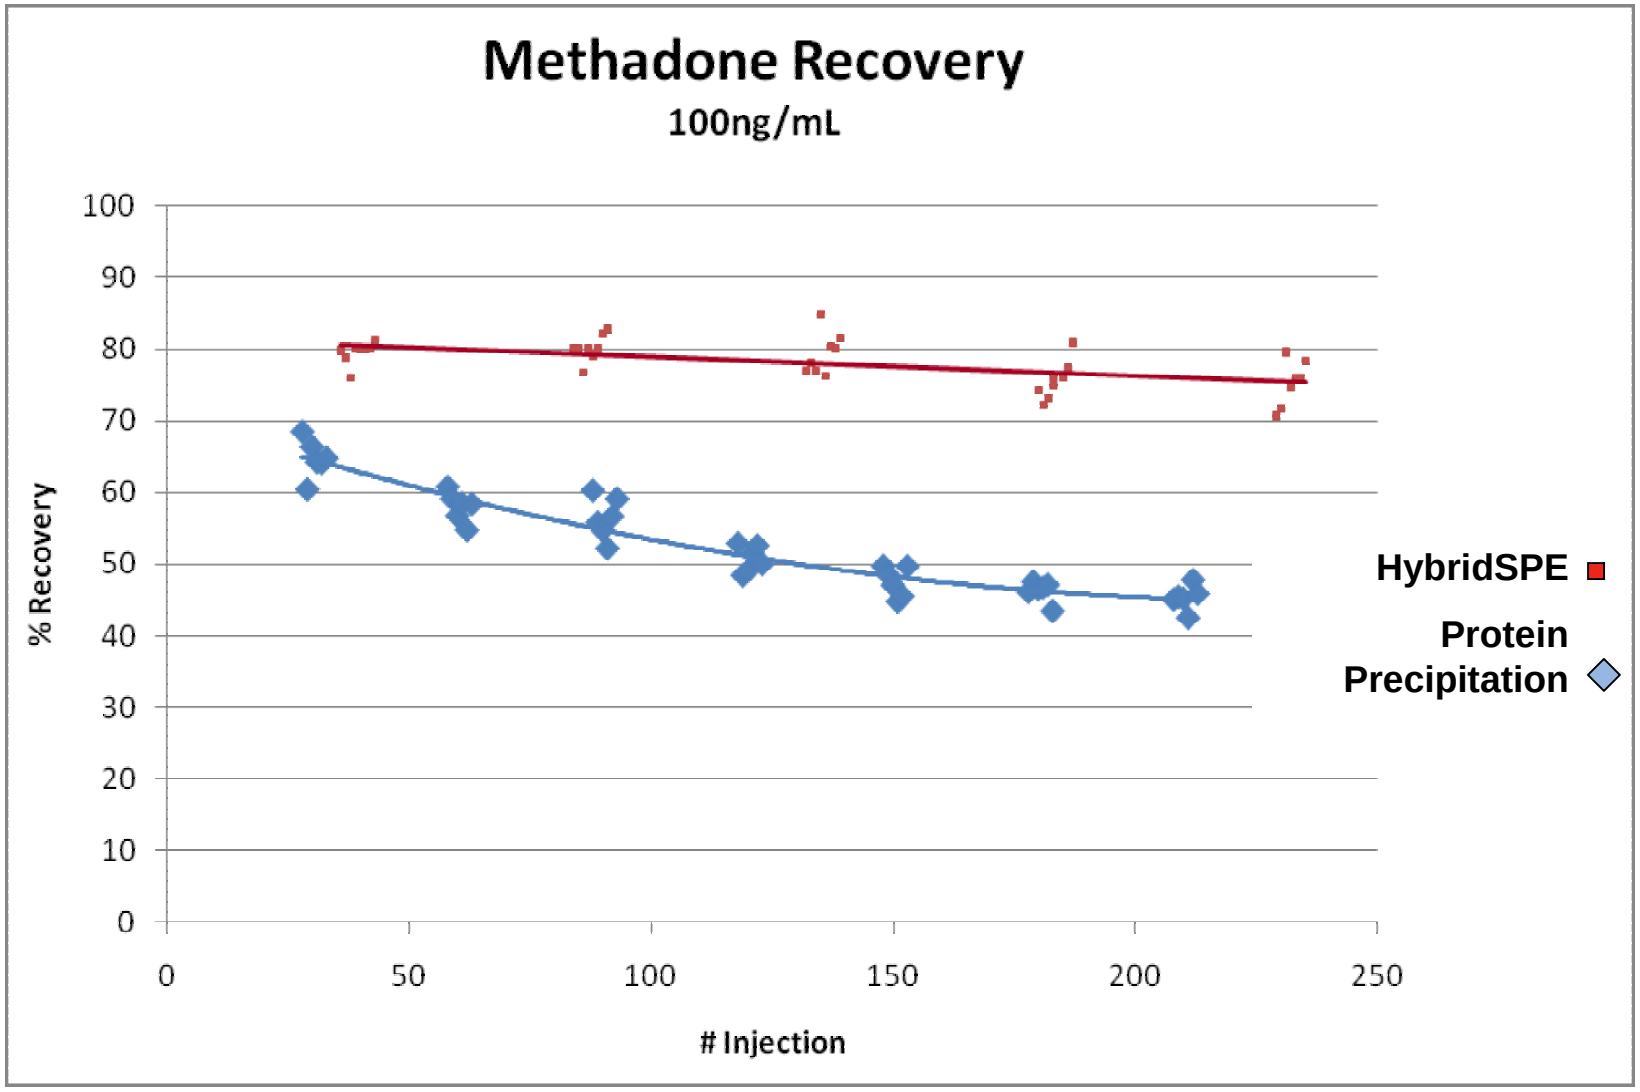

© 2010 Sigma-Aldrich Co. All rights reserved.

SIGMA-ALDRICH®

Conclusions

- Phospholipid buildup and resulting matrix ionization effect was demonstrated when performing standard protein precipitation techniques.
- HybridSPE-Small Volume plate demonstrated high recovery of methadone and associated metabolites across the concentration range along with depletion of proteins and phospholipids from the plasma samples.
- Unique approach to processing small volume samples enable a high degree of matrix removal when dealing with minimal plasma volumes.
- Utilizing the zirconia-Si particles as a sample preparation media, phospholipid matrix interference was selectively bound to the particle via Lewis acid/base interaction resulting in high degree of phospholipid removal.
- Consideration towards sample matrix… fast chromatographic separation do not always translate to fast bioanalytical methods.

© 2010 Sigma-Aldrich Co. All rights reserved.